

medartis®

PRECISION IN FIXATION

PRODUCT INFORMATION

Coronoid Plates 2.0




APTUS®
Elbow

APTUS® Elbow Coronoid Plates 2.0

Stable fixation for coronoid fractures
Anatomical fit and angular stable


Plate Features

- Anatomical plate design for left and right
- TriLock – multidirectional ($\pm 15^\circ$) and angular stable locking technology
- Screw angle can be adapted intraoperatively and fracture fragments can be fine-tuned
- Integrated and compatible with the existing APTUS Elbow System 2.0
- K-wire holes for temporary plate and fragment fixation
- Bending to be contoured to the individual anatomy
- Combination of 2.0 TriLock screws and cortical screws

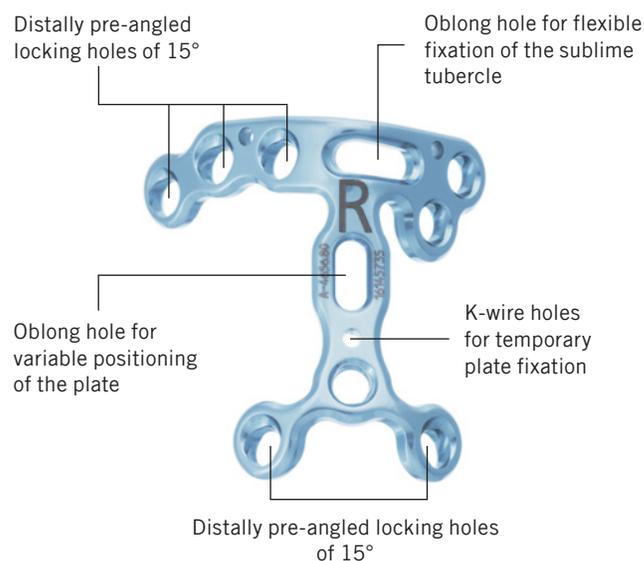

Clinical Benefits


- Buttressing and fixation of the sublime tubercle for restoration of the elbow stability (indirect refixation of the medial collateral ligament)
- For the anterior as well as the anteromedial variation of the Hotchkiss approach
- Possibility of subchondral screw placement
- Proximal oblong hole increases flexibility of screw placement and angulation
- Low plate profile, rounded edges and a smooth surface for soft tissue protection
- Uniform screw diameter of 2.0 mm

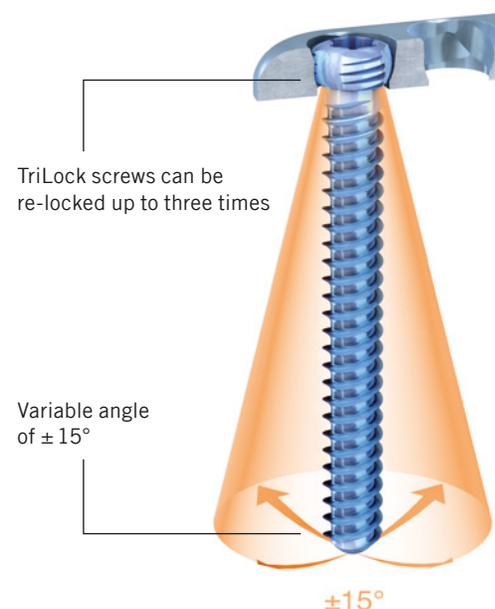

Ordering Information


2.0 TriLock Coronoid Plates

Material: Titanium (ASTM F67)
Plate thickness: 1.6 mm

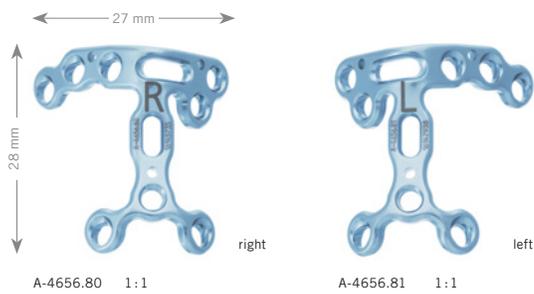

Art. No.	Description	Holes	Pieces/Pkg
A-4656.80	right	10	1
A-4656.81	left	10	1

Coronoid Module

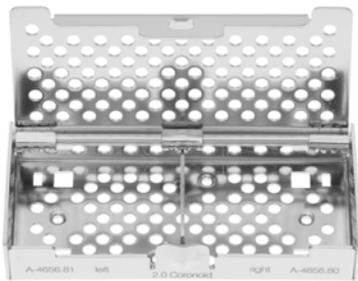

Art. No.	Description	Pieces/Pkg
A-6530.1	for A-6530	1

ELBOW-03000006_v1 / © 2019-08, Medartis AG, Switzerland. All technical data subject to alteration.

MANUFACTURER & HEADQUARTERS

Medartis AG | Hochbergerstrasse 60E | 4057 Basel/Switzerland
P +41 61 633 34 34 | F +41 61 633 34 00 | www.medartis.com

SUBSIDIARIES

Australia | Austria | Brazil | France | Germany | Japan | Mexico | New Zealand | Poland | UK | USA

For detailed information regarding our subsidiaries and distributors, please visit www.medartis.com



Disclaimer: This information is intended to demonstrate the Medartis portfolio of medical devices. A surgeon must always rely on her or his own professional clinical judgement when deciding whether to use a particular product when treating a particular patient. Medartis is not giving any medical advice. The devices may not be available in all countries due to registration and/or medical practices. For further questions, please contact your Medartis representative (www.medartis.com). This information contains CE-marked products.
For US only: Federal law restricts this device to sale by or on the order of a physician.